

DOI: [10.29026/oea.2024.240074](https://doi.org/10.29026/oea.2024.240074)

Laser-induced stretchable bioelectronic interfaces by frozen exfoliation

Xiaowei Li*

Highly stretchable laser-induced graphene—hydrogel film interfaces in flexible electronic materials are fabricated by frozen exfoliation, and exhibit high stretchability, durability, and design flexibility. This technology offers an advanced technological pathway for manufacturing highly flexible substrates. They can be utilized in numerous complex surface applications, providing an advanced technological pathway for manufacturing highly flexible substrates in the future.

Li XW. Laser-induced stretchable bioelectronic interfaces by frozen exfoliation. *Opto-Electron Adv* 7, 240074 (2024).

In recent years, the rapid advancement of flexible and stretchable electronics has been fueled by their soft and thin characteristics, biocompatibility, and long-term stability^{1–4}. The stretchability of flexible materials^{5–7} is critical to the mechanical and electrical performance stability of flexible electronics when conformally adhered to free-form surfaces, and this has attracted widespread attention. Graphene, due to its exceptional electromechanical properties, has been widely applied in flexible electronic systems^{8–11}. Recently, the synthesis and processing method of inducing graphene from aromatic polymers through laser irradiation has made the one-step fabrication and patterning of graphene devices possible^{12–14}. By controlling the temperature value of the irradiating laser, selective polymer graphitization can be achieved, resulting in laser-induced graphene (LIG) with porous conductive characteristics, which possesses high sensitivity and low resistance. They can conformably and compliantly adhere to irregular organs such as the skin^{15,16}, brain^{17,18}, and heart^{19,20}, and have been extensively applied in multiple scenarios of bioelectronics.

Although LIG has been used in diverse flexible electronic devices, it still remains bound to the precursor

polymers, limiting its stretchability and conformability in wearable and implantable applications. This issue has limited their broader industrial applications. Researchers have been devoted to achieving a highly mechanically stable interface between highly conductive electrode materials and highly flexible materials, which is a central challenge in the manufacturing of flexible electronics.

In a recent paper published in *Nature Electronics*²¹, Prof. Kaichen Xu and Prof. Zhen Gu et al. from Zhejiang University proposed a thin elastic conductive nanocomposite based on LIG micropatterns, which is realized by a cryogenic transfer approach with an ultrathin and adhesive polyvinyl alcohol (PVA)–phytic acid (PA)–honey (PPH) hydrogel with the thickness of 1–1.5 μm . This approach has achieved 110% intrinsic stretchability and 220% structural optimization, which realize an improvement of more than fivefold over the previously reported flexible electrode materials composed of brittle LIG and polydimethylsiloxane (PDMS). The graphene-hydrogel nanocomposite films prepared in this way possess excellent sensing performance, antibacterial properties, biocompatibility, and high stretchability, which are

Laser Micro/Nano Fabrication Laboratory, School of Mechanical Engineering, Beijing Institute of Technology, Beijing 100081, China.

*Correspondence: XW Li, E-mail: lixiaowei@bit.edu.cn

Received: 2 April 2024; Accepted: 7 April 2024; Published online: 4 June 2024



Open Access This article is licensed under a Creative Commons Attribution 4.0 International License.

To view a copy of this license, visit <http://creativecommons.org/licenses/by/4.0/>.

© The Author(s) 2024. Published by Institute of Optics and Electronics, Chinese Academy of Sciences.

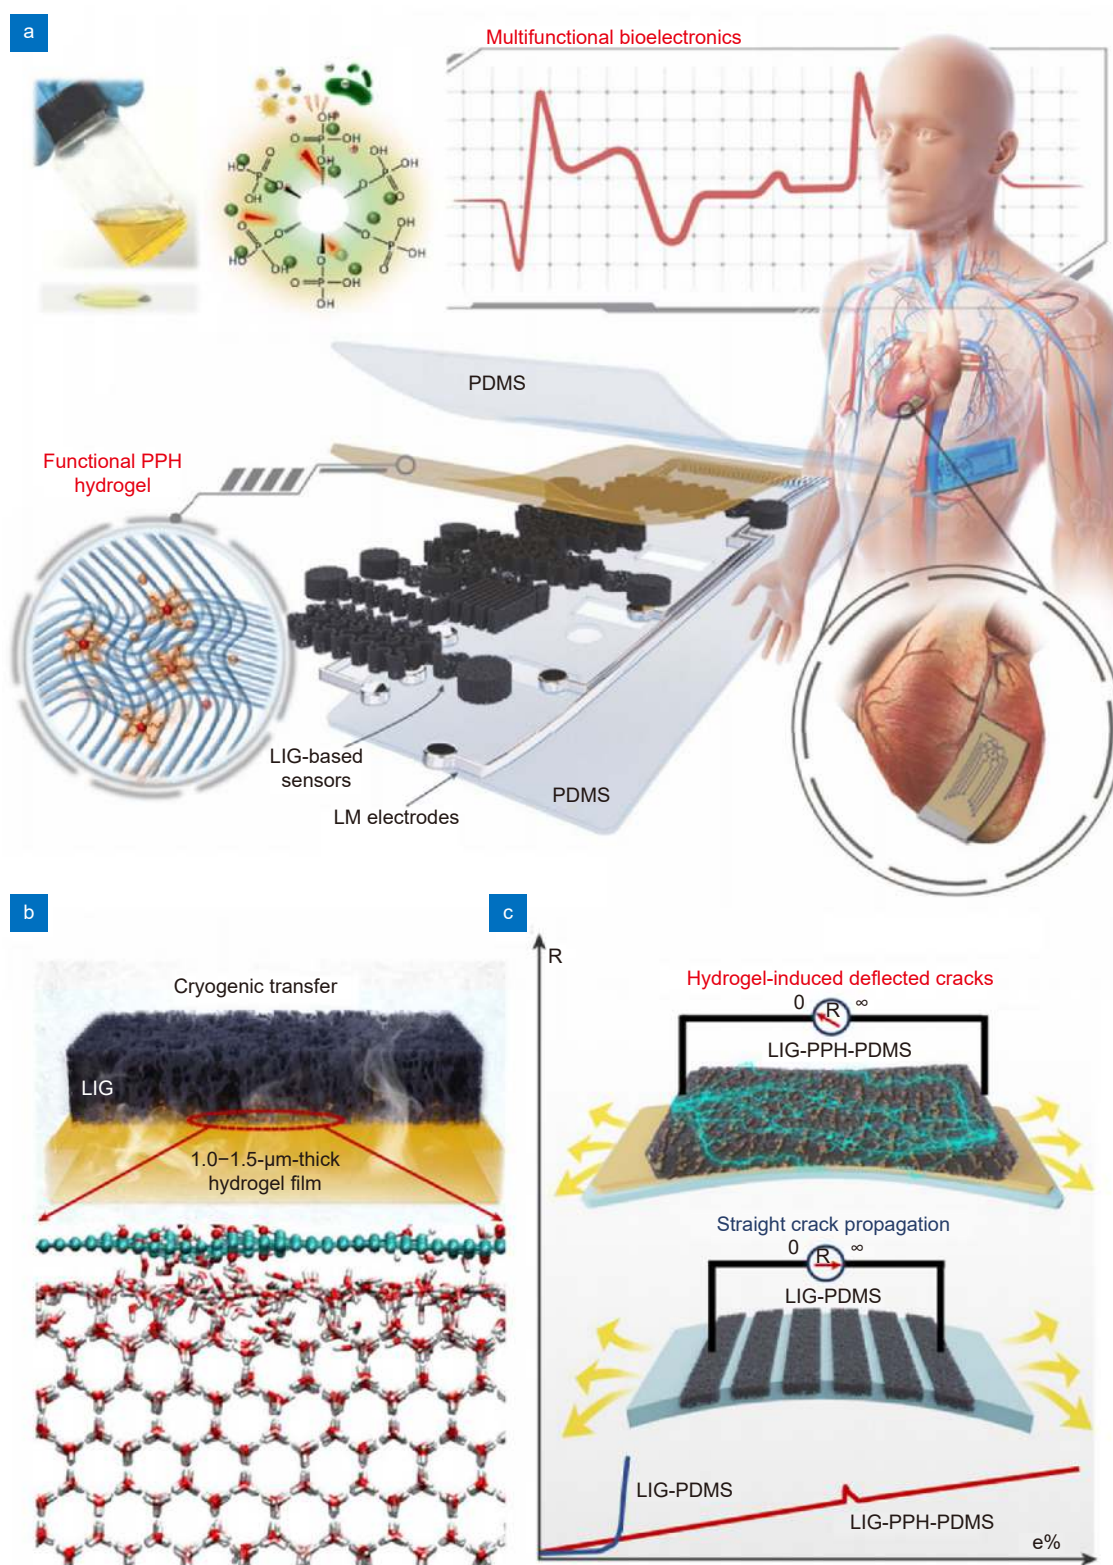


Fig. 1 | The schematic of the design scheme of stretchable graphene–hydrogel nanocomposites¹⁷

crucial for skin patches and implantable electronic devices.

Figure 1 shows the schematic of the highly stretchable flexible electronic material preparation technology based

on high-strength bonding of LIG and PPH hydrogel. The key aspects of this technology mainly include two parts. First, the high-stability transfer scheme allows for low-temperature peeling of LIG onto the PPH hydrogel with

low Young's modulus, high adhesiveness, and antibacterial performance. On the one hand, low-temperature interfacial electrostatic interactions enhance the interfacial binding energy between crystalline water molecules in the hydrogel. At the same time, the low temperature causes the gel layer to expand in volume, allowing the porous LIG part to embed into the PPH film. This leads to the formation of interlocking structures with high mechanical stability, which improves the robustness of the composite material. Second, compared with traditional LIG-PDMS conductive materials, the ultra-thin PPH provides the higher adhesion due to the dipole effect of $-P=O$, $-C=O$, $-C-F$ and $-CF_3$ groups, which results in the deflected fractures with ductile behaviours, and can provide out-of-plane points of contact to connect the fractured LIG film, thus enhancing the intrinsic conductive stretchability of the nanocomposite material. Based on the aforementioned fabrication technology, a further development involves constructing integrated multifunctional sensing skin patches that include strain sensors, temperature sensors, humidity sensors, and electrocardiogram (ECG) sensors, as well as an array of strain sensors adhered to the surface of the heart for in-body applications. This facilitates the monitoring of near-death signals caused by arrhythmias, demonstrating practical applications of the sensors. It also proves the enhanced conformability of the fabricated flexible sensors to complex surfaces and the improvement of their signal stability.

Based on the low-temperature transfer scheme for nanocomposite material preparation, there is a significant advantage in terms of stretchability and mechanical strength, and there is also great potential for further development. The design and fabrication of three-dimensional micro/nanostructures and circuit morphologies can further enhance the sensitivity of the sensing system^{22–24}. Moreover, laser fabrication methods, such as LIG, necessitate further investigation into their scalability for the production of large-area electronics and bioelectronics. Advancing this research could elevate these technologies to the scalability of other fabrication strategies, such as printed electronics using two-dimensional materials²⁵. For example, spatial-temporal shaping femtosecond laser can achieve flexible control of the surface micro-nano structures and efficient preparation. It has been reported that femtosecond laser-induced graphene possesses the smaller dimensions and higher electrical conductivity, allowing for the preparation of LIG with higher precision^{12,26}. In summary, the scheme presented

in this paper for low-temperature transfer of LIG to ultra-thin flexible substrates exhibits high stretchability, high robustness, and high design flexibility, providing an advanced technical pathway for the future fabrication of highly flexible substrates towards many complex surface applications, such as smart brain patches, soft wound patches, and electrical stimulation for muscle treatment.

References

- Zhong DL, Wu C, Jiang YW et al. High-speed and large-scale intrinsically stretchable integrated circuits. *Nature* **627**, 313–320 (2024).
- Xue TY, Fan BJ, Jiang KJ et al. Self-healing ion-conducting elastomer towards record efficient flexible perovskite solar cells with excellent recoverable mechanical stability. *Energy Environ Sci* **17**, 2621–2630 (2024).
- Manjakkal L, Pereira L, Kumi Barimah E et al. Multifunctional flexible and stretchable electrochromic energy storage devices. *Prog Mater Sci* **142**, 101244 (2024).
- Cui SY, Lu YY, Kong DP et al. Laser direct writing of Ga₂O₃/liquid metal-based flexible humidity sensors. *Opto-Electron Adv* **6**, 220172 (2023).
- Yi JQ, Zou GJ, Huang JP et al. Water-responsive supercontractile polymer films for bioelectronic interfaces. *Nature* **624**, 295–302 (2023).
- Won D, Bang J, Choi SH et al. Transparent electronics for wearable electronics application. *Chem Rev* **123**, 9982–10078 (2023).
- Liu W, Zhang C, Alessandri R et al. High-efficiency stretchable light-emitting polymers from thermally activated delayed fluorescence. *Nat Mater* **22**, 737–745 (2023).
- Kireev D, Sel K, Ibrahim B et al. Continuous cuffless monitoring of arterial blood pressure via graphene bioimpedance tattoos. *Nat Nanotechnol* **17**, 864–870 (2022).
- Törmä P, Peotta S, Bernevig BA. Superconductivity, superfluidity and quantum geometry in twisted multilayer systems. *Nat Rev Phys* **4**, 528–542 (2022).
- Sun MW, Cui SY, Wang ZZ et al. A laser-engraved wearable gait recognition sensor system for exoskeleton robots. *Microssyst Nanoeng* **10** (2024).
- Xu KC, Li QA, Lu YY et al. Laser Direct Writing of Flexible Thermal Flow Sensors. *Nano Letters* **23**, 10317–10325 (2023).
- Le TSD, Park S, An JN et al. Ultrafast laser pulses enable one-step graphene patterning on woods and leaves for green electronics. *Adv Funct Mater* **29**, 1902771 (2019).
- Lin J, Peng ZW, Liu YY et al. Laser-induced porous graphene films from commercial polymers. *Nat Commun* **5**, 5714 (2014).
- Cai ZM, Kuang CF, Yang HY et al. Hybrid Laser Manufacturing and Applications in Flexible Micro - Nano Sensors (Invited). *Chinese Journal of Lasers* **51**, 0402403 (2024).
- Cao LT, Liu Q, Ren J et al. Electro-blown spun silk/graphene nanoionotronic skin for multifunctional fire protection and alarm. *Adv Mater* **33**, 2102500 (2021).
- He P, Du T, Zhao KR et al. Lightweight 3D graphene metamaterials with tunable negative thermal expansion. *Adv Mater* **35**, 2208562 (2023).
- Ramezani M, Kim JH, Liu X et al. High-density transparent

- graphene arrays for predicting cellular calcium activity at depth from surface potential recordings. *Nat Nanotechnol* **19**, 504–513 (2024).
18. Bonaccini Callia A, Masvidal-Codina E, Smith TM et al. Full-bandwidth electrophysiology of seizures and epileptiform activity enabled by flexible graphene microtransistor depth neural probes. *Nat Nanotechnol* **17**, 301–309 (2022).
 19. Lin ZX, Kireev D, Liu N et al. Graphene biointerface for cardiac arrhythmia diagnosis and treatment. *Adv Mater* **35**, 2212190 (2023).
 20. Liu Y, Zhou H, Zhou WX et al. Biocompatible, high-performance, wet-adhesive, stretchable all-hydrogel supercapacitor implant based on PANI@rGO/mxenes electrode and hydrogel electrolyte. *Adv Energy Mater* **11**, 2101329 (2021).
 21. Lu YY, Yang G, Wang SQ et al. Stretchable graphene–hydrogel interfaces for wearable and implantable bioelectronics. *Nat Electron* **7**, 51–65 (2024).
 22. Hu JX, Gou J, Yang M et al. Room-temperature colossal magnetoresistance in terraced single-layer graphene. *Adv Mater* **32**, 2002201 (2020).
 23. Yi P, Fu XP, Liu Y et al. Triboelectric active pressure sensor with ultrabroad linearity range by femtosecond laser shaping based on electrons dynamics control. *Nano Energy* **113**, 108592 (2023).
 24. Liu Y, Li XW, Huang J et al. High-uniformity submicron gratings with tunable periods fabricated through femtosecond laser-assisted molding technology for deformation detection. *ACS Appl Mater Interfaces* **14**, 16911–16919 (2022).
 25. Pinilla S, Coelho J, Li K et al. Two-dimensional material inks. *Nat Rev Mater* **7**, 717–735 (2022).
 26. Zou TT, Zhao B, Xin W et al. High-speed femtosecond laser plasmonic lithography and reduction of graphene oxide for anisotropic photoresponse. *Light Sci Appl* **9**, 69 (2020).



Scan for Article PDF